Breezi
How to Fit

MADE BY BES HEALTHCARE

Millie Mova (Not applicable for Breezi MAX: use ByBESIn017M)

4mm Hex

3mm 7mm

Pozidrive #2

10mm

P x1

A X2 B X2



4x25(mm)

C X2 D X2 E X4 F X2 K X2

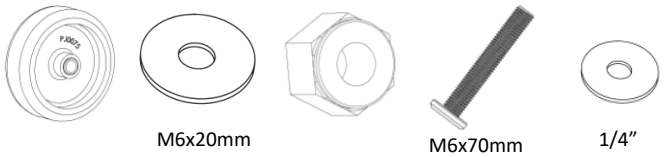

M6x20mm M6x70mm 1/4”

G X1 H X2 J X2 D X2 E X2 K X2

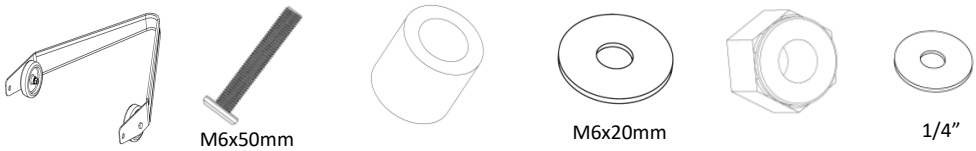

M6x50mm M6x20mm 1/4”

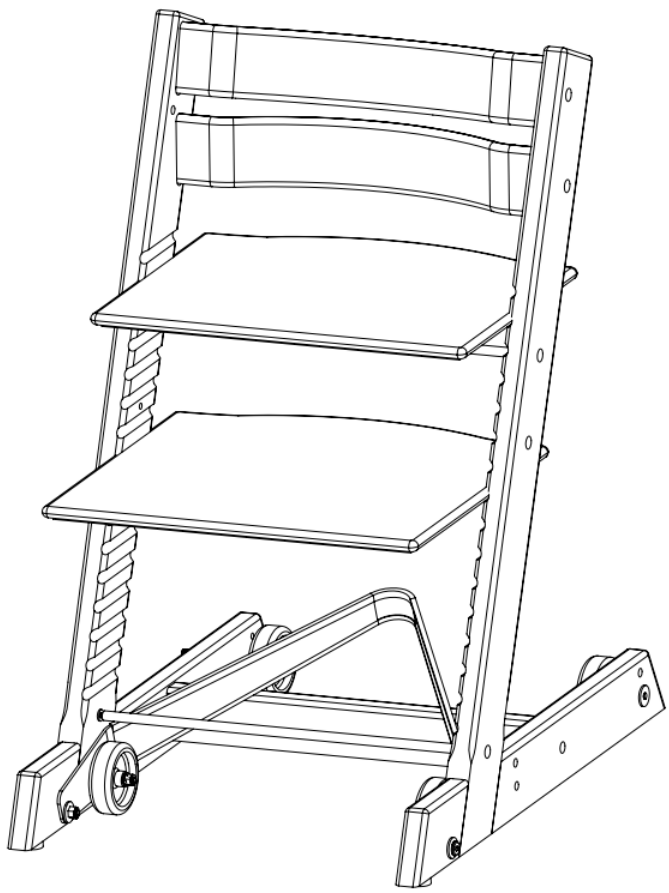

BES Healthcare Ltd 0117 966 6761 info@beshealthcare.net beshealthcare.net

131 South Liberty Lane, Ashton Vale, Bristol, BS3 2SZ UK *© 2022*

CE

BHTA British Healthcare Trades Association

1 X2

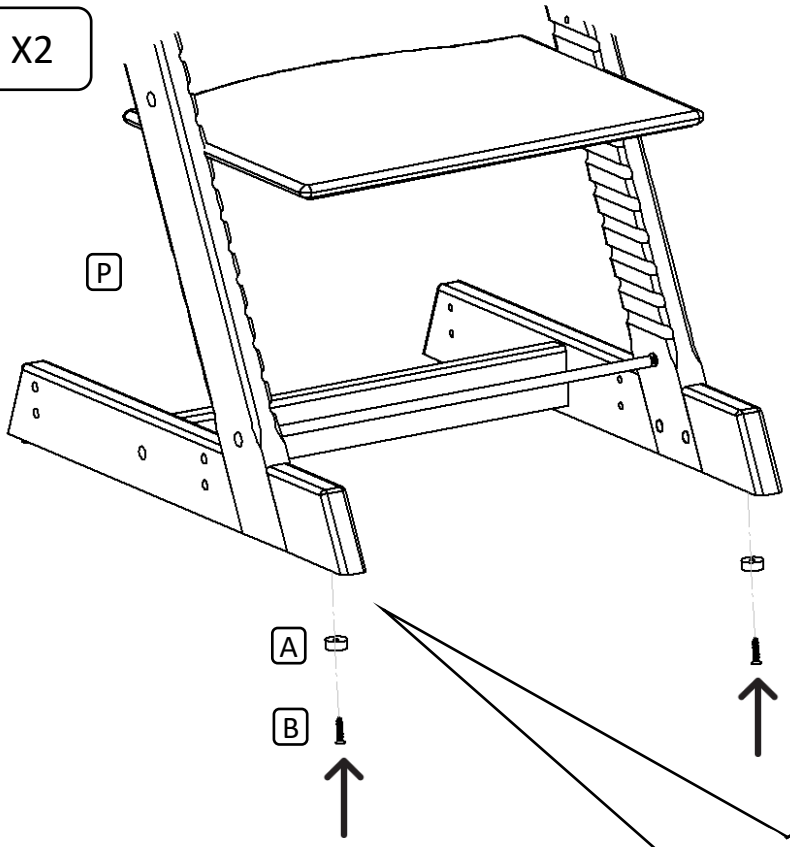

1.1

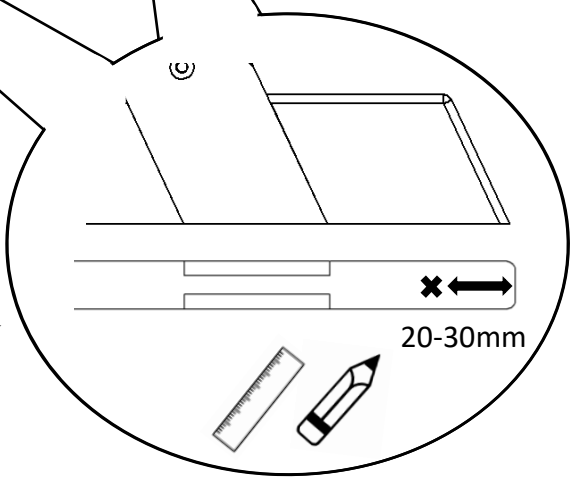

1.2

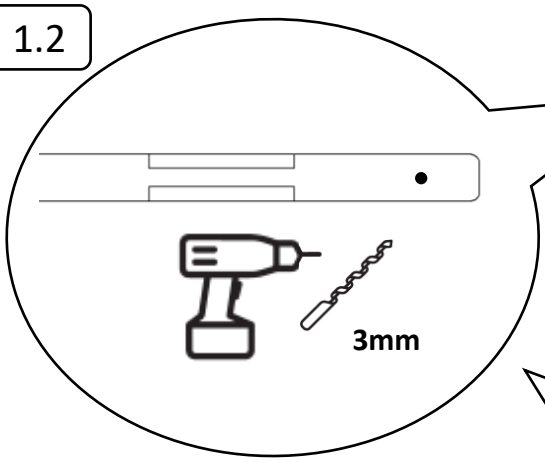

1.3

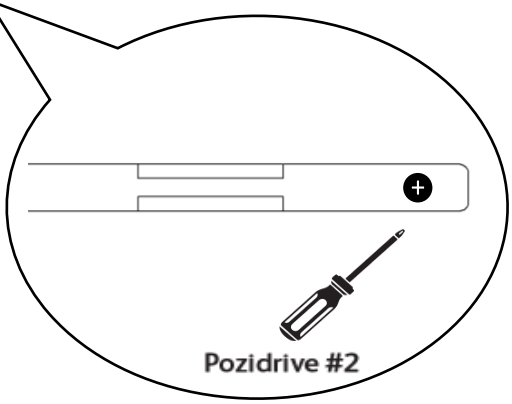

BES Healthcare Ltd 0117 966 6761 info@beshealthcare.net beshealthcare.net

131 South Liberty Lane, Ashton Vale, Bristol, BS3 2SZ UK *© 2022*

CE

BHTA British Healthcare Trades Association

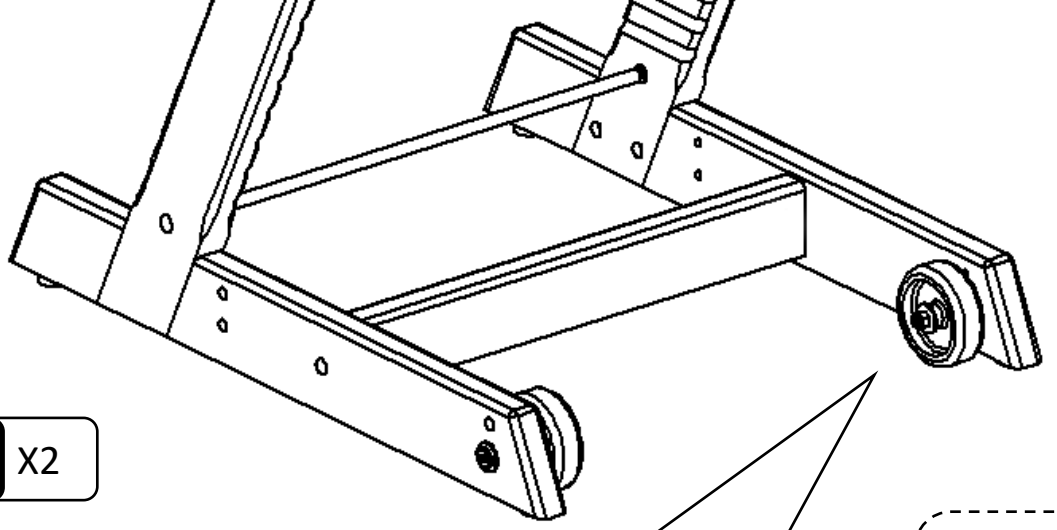

2 X2

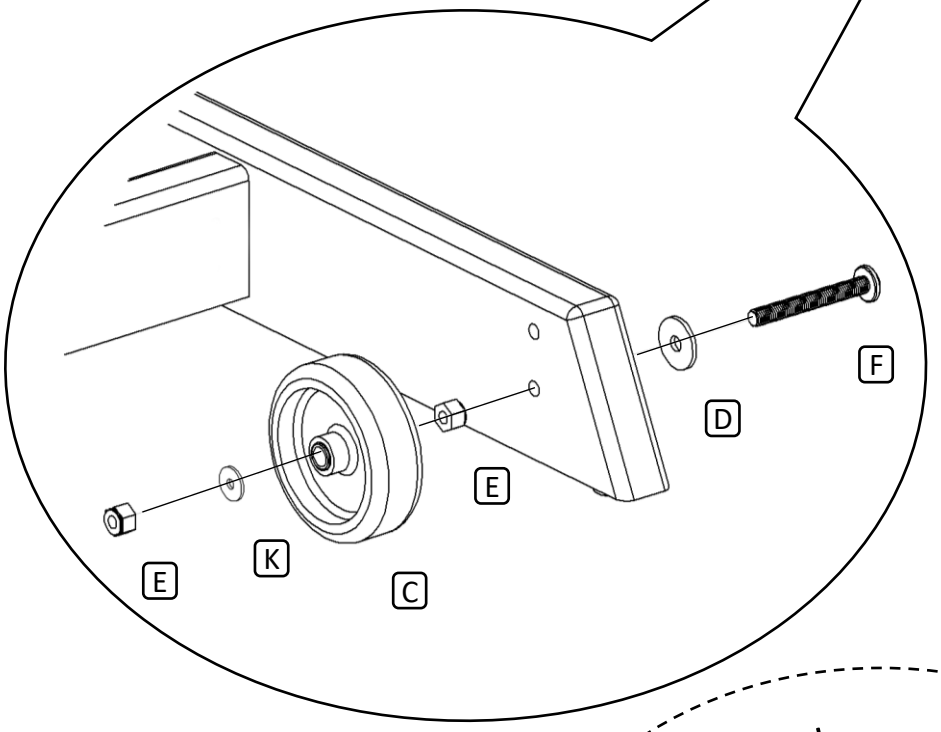



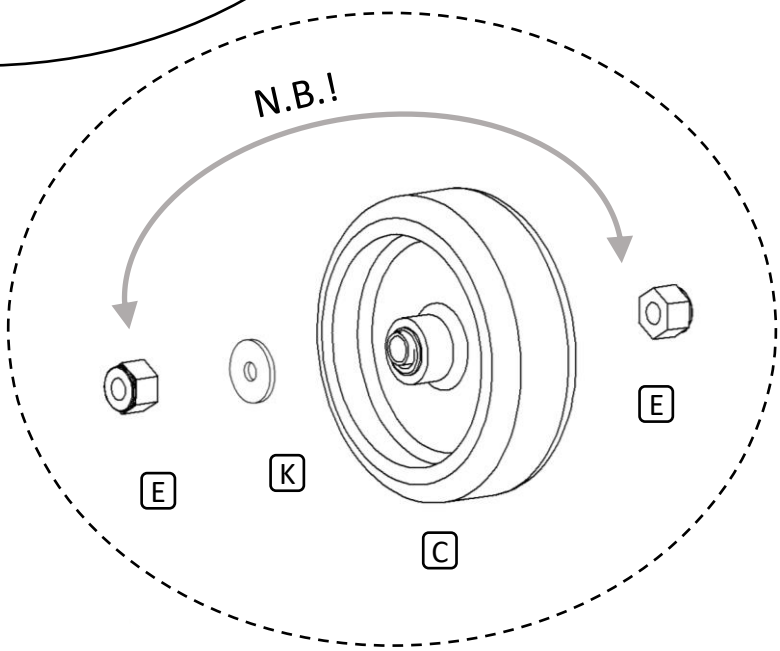

BES Healthcare Ltd 0117 966 6761 info@beshealthcare.net beshealthcare.net

131 South Liberty Lane, Ashton Vale, Bristol, BS3 2SZ UK *© 2022*

CE

BHTA British Healthcare Trades Association

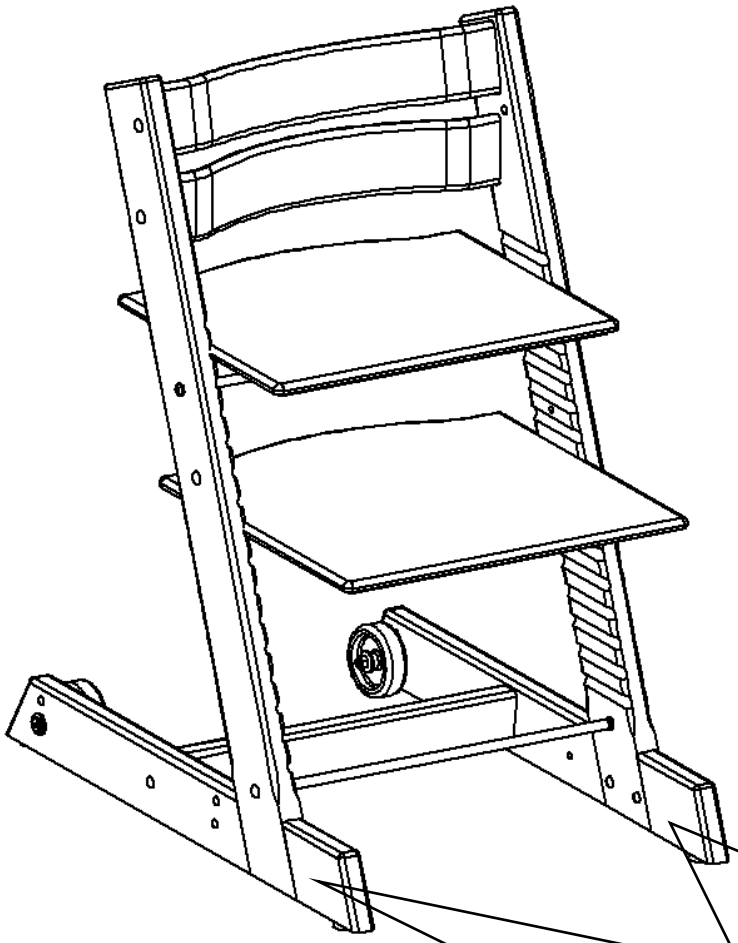

3 X2

3.1

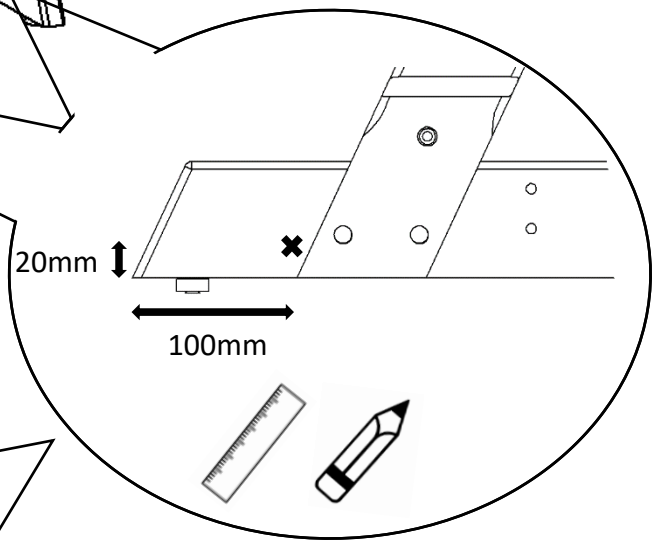

3.2

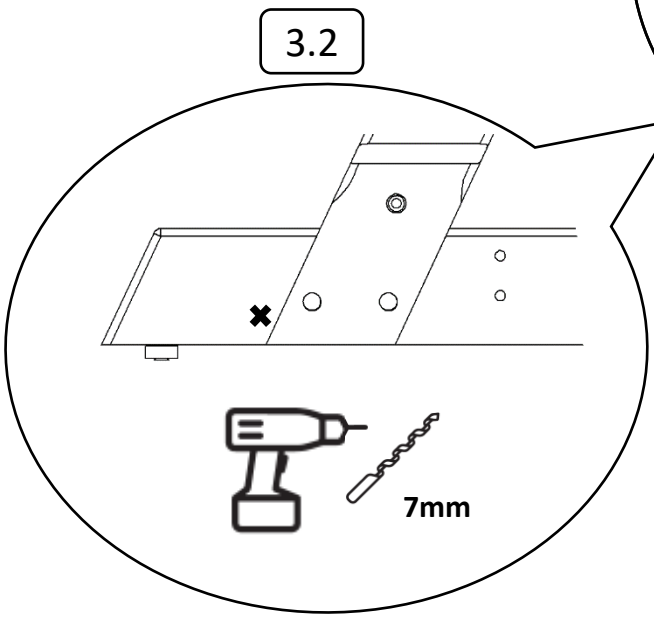

BES Healthcare Ltd 0117 966 6761 info@beshealthcare.net beshealthcare.net

131 South Liberty Lane, Ashton Vale, Bristol, BS3 2SZ UK *© 2022*

CE

BHTA British Healthcare Trades Association

4 X2

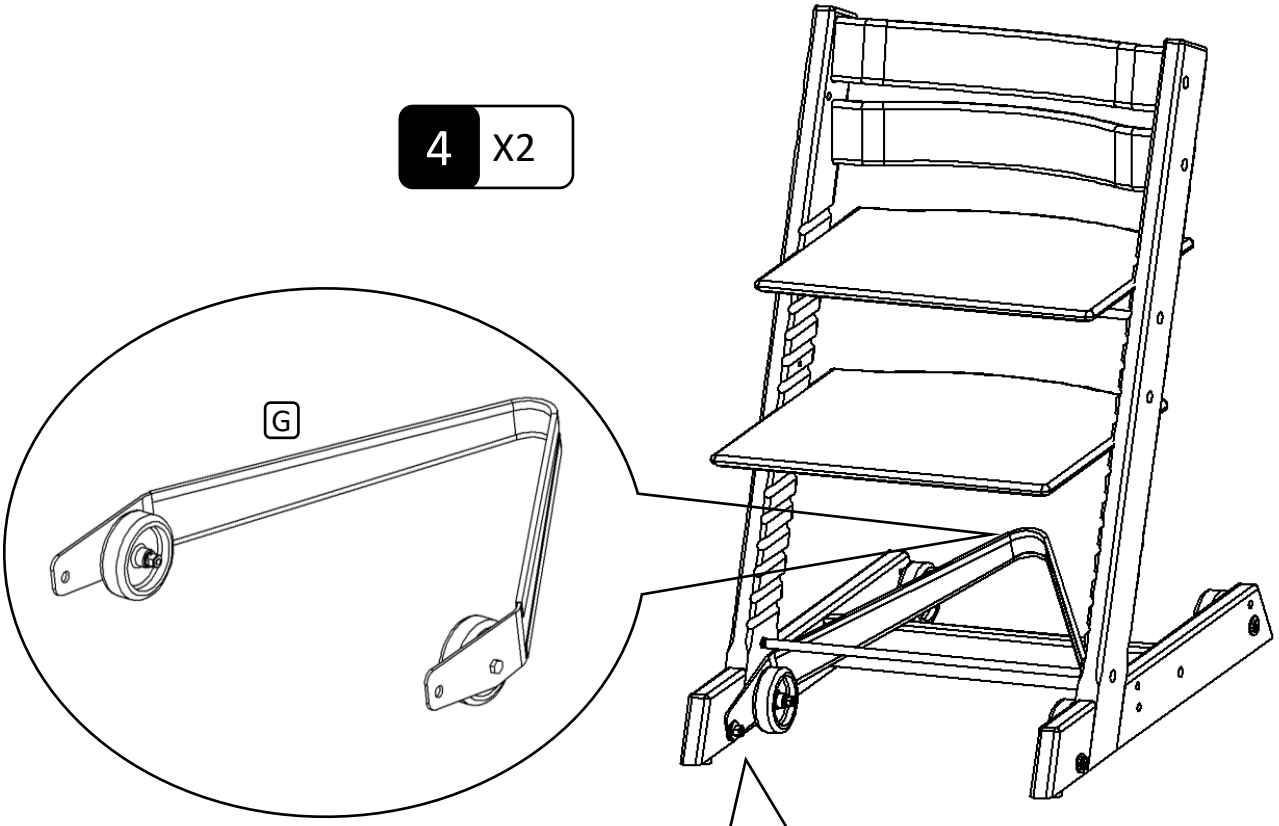





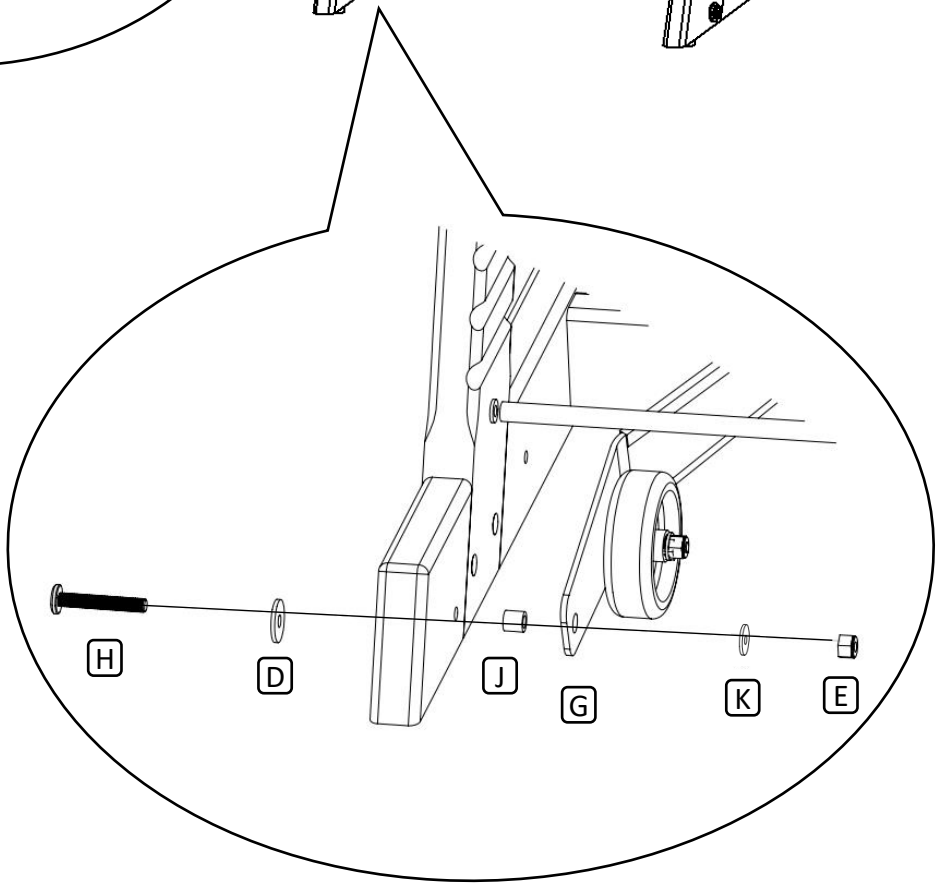

BES Healthcare Ltd 0117 966 6761 info@beshealthcare.net beshealthcare.net

131 South Liberty Lane, Ashton Vale, Bristol, BS3 2SZ UK *© 2022*